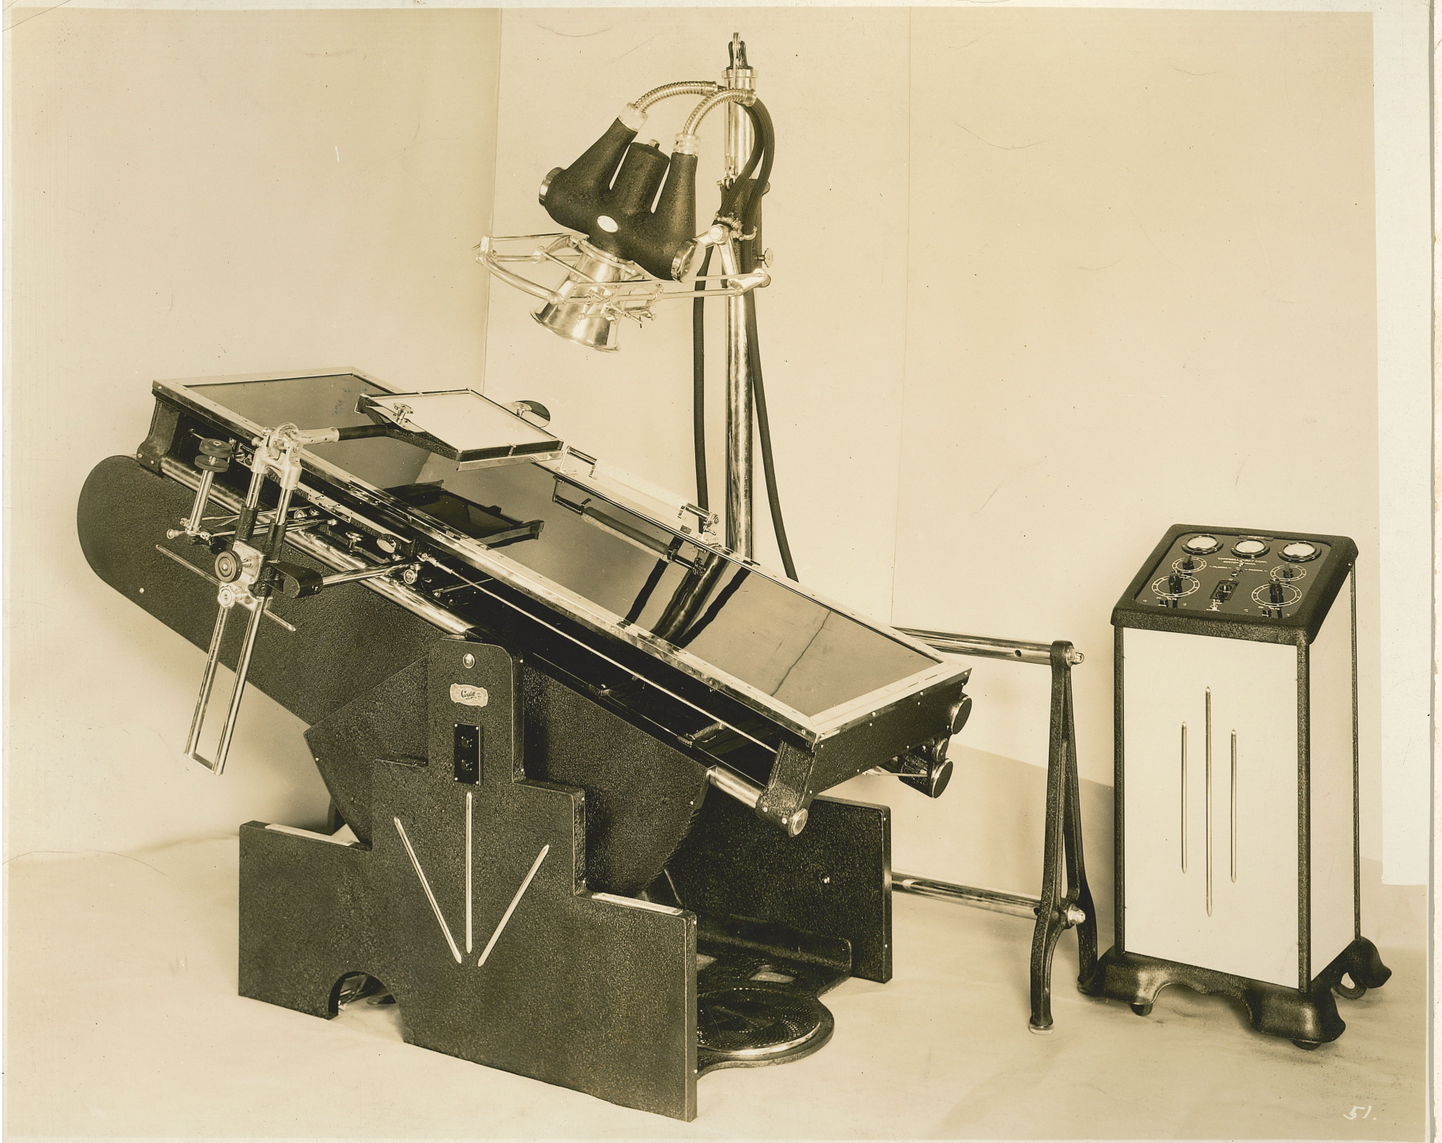

Clinix

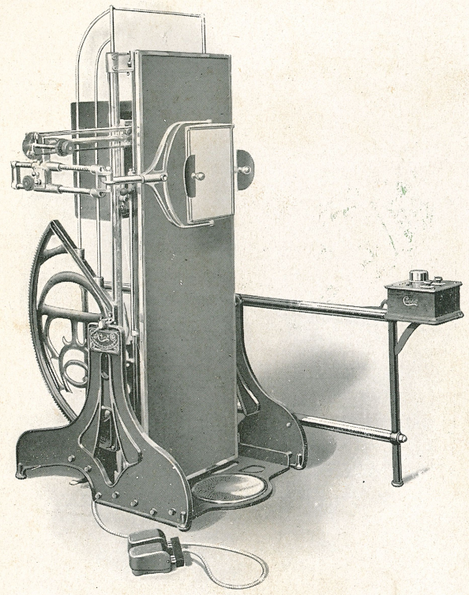

CLINIX IN VERTICAL POSITION

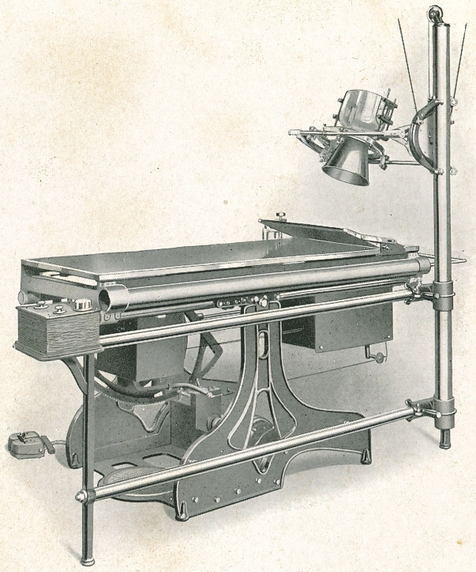

CLINIX IN HORIZONTAL POSITION
Rear view showing Transformer and Connections

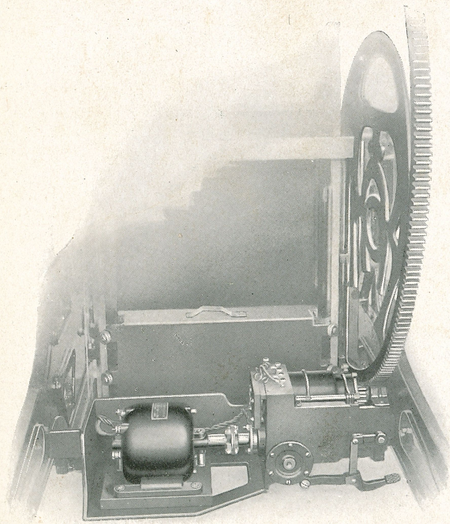

CLINIX MOTOR DRIVE AND TRANSMISSION

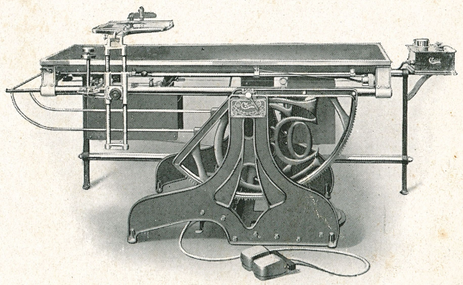

CLINIX IN HORIZONTAL POSITION
Operating Side

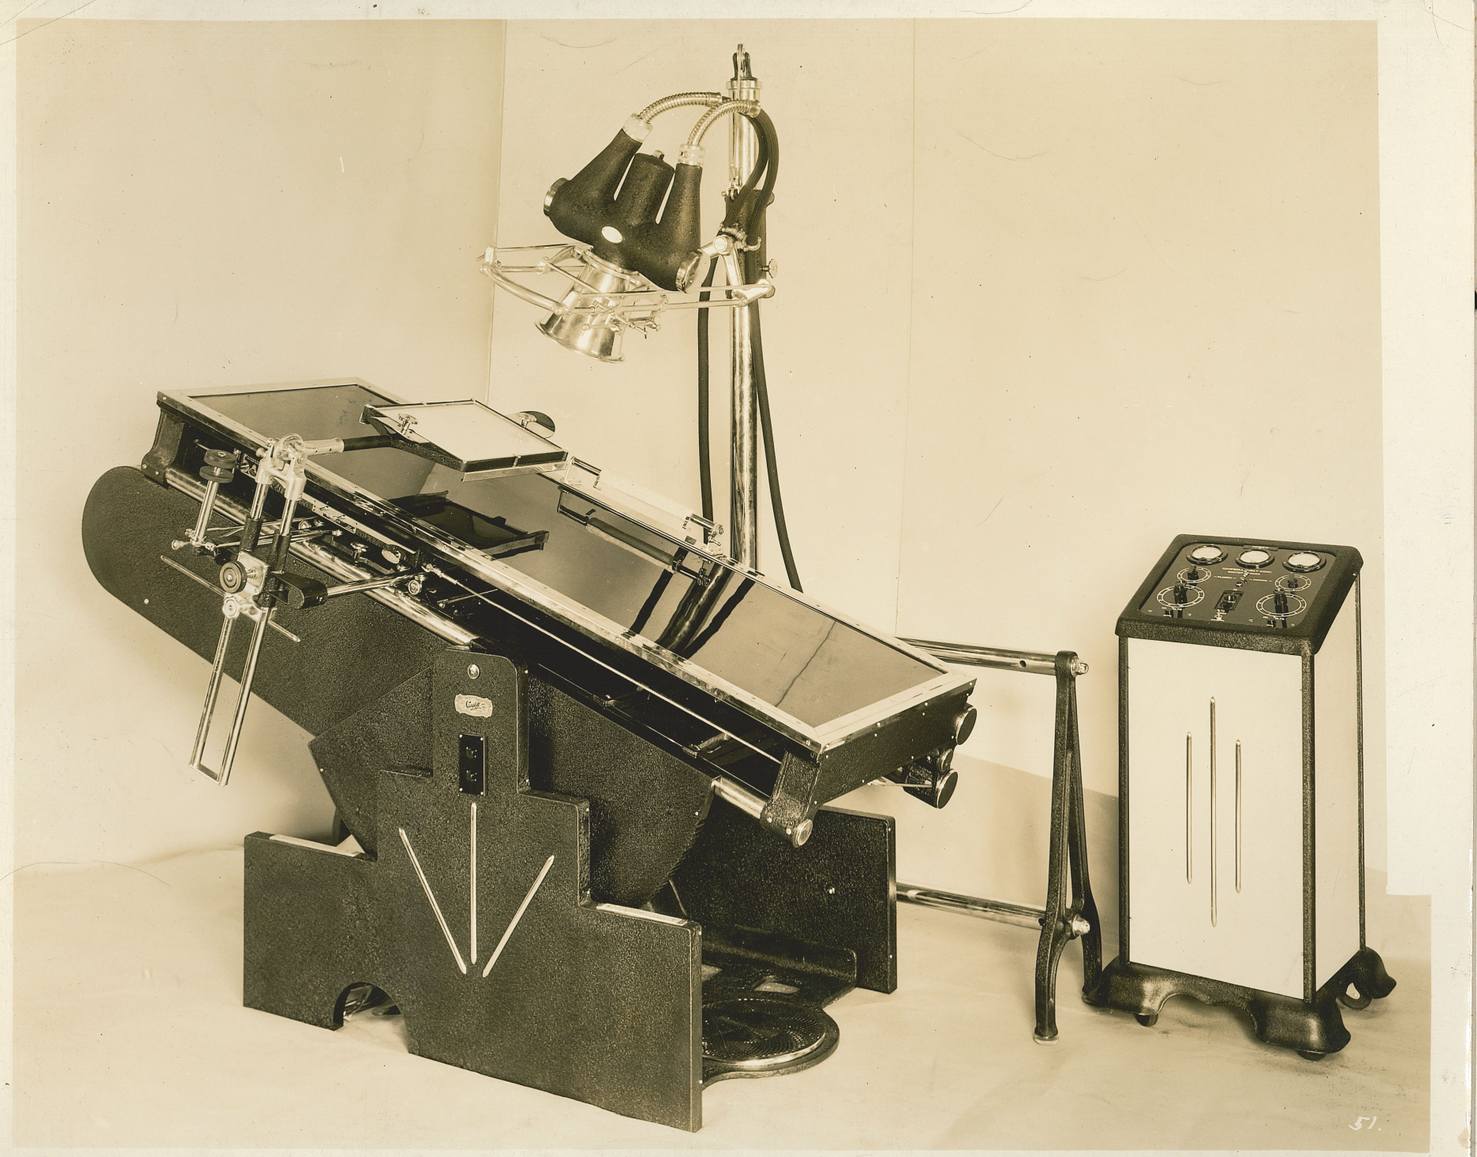

TRADE MARK

Clinix

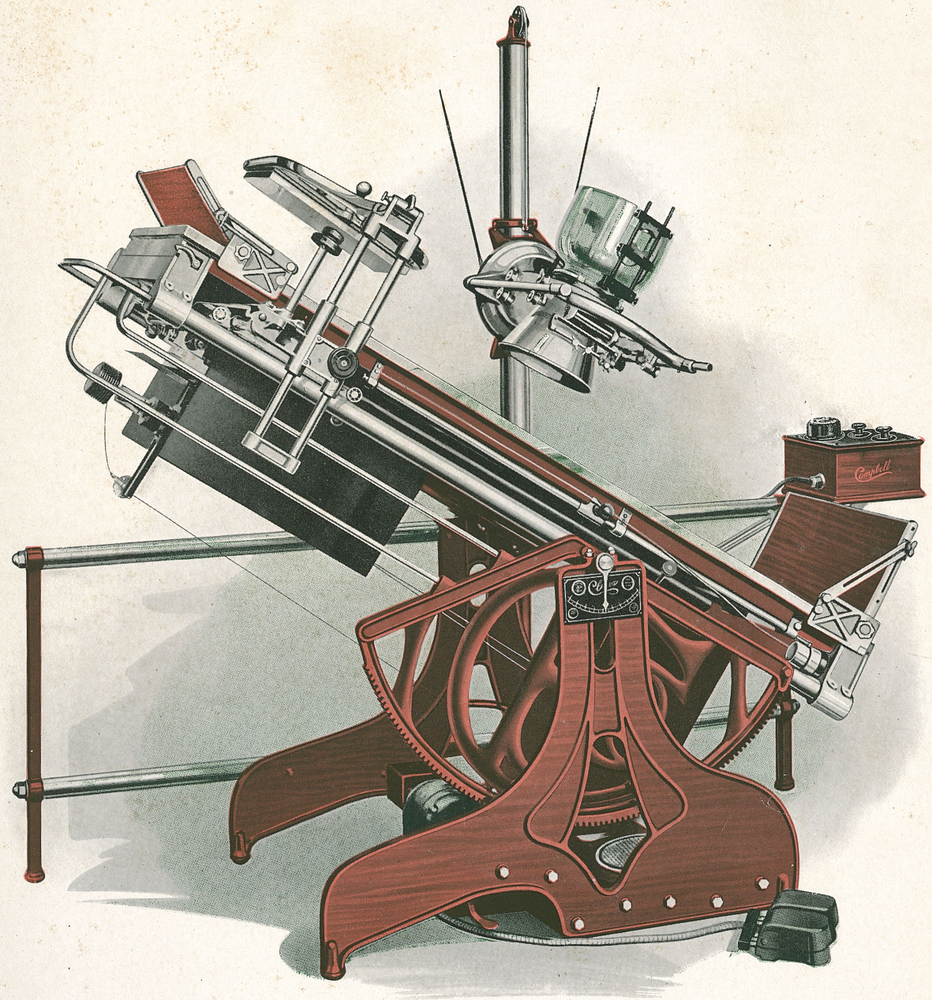

Campbell "Clinix" X-ray Plant

Tube Tilt Table. Motor Driven. Transformer attached to under side of table.
Also furnished with Transformer mounted on top of Tube Stand.
Both High Tension Transformers operated by the one Auto Transformer Control Case.
1 to 30 Milliamperes, 2 to 5-inch Spark Gap.

U. S. Patents
December 19, 1911; April 22, 1913; February 29, 1916;
August 7, 1917. Foreign Patents.
Other Patents Pending.

Cat. No. 2087